8000R

SpO_2 Forehead Sensor

Quick Start Guide

NONIN

1 **Remove adhesive backing** from one horseshoe shaped adhesive ring.

2 **Press the clear holder on the ring** so a slot is open for the sensor cable. Remove from the card.

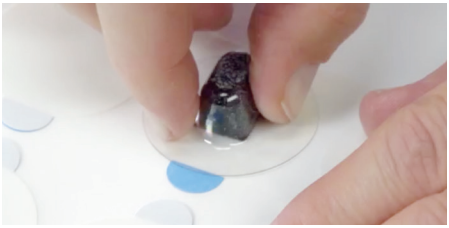

3 **Press a clean 8000R sensor into the grey foam,** with the emitter/detector facing **away** from the foam, and cable in slot.

4 **Wipe the forehead with an alcohol swab.** Allow to dry.

5 **Gently press on the forehead.**

6 **Apply a piece of medical tape** to keep it firmly in place.

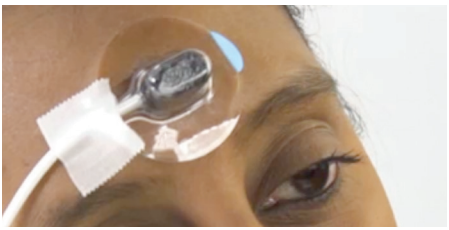

Additional Guidance

Check sensor position and skin at site every 6 to 8 hours.

If signal quality is low on the oximeter:

1. Check connection at oximeter.
2. Check that forehead is warm and has good blood flow.
3. Use another location.

Clean sensor between patients or as needed:

1. **Remove and discard the used 8000H holder.**
2. **Wipe all patient contact surfaces with a soft cloth dampened with a 10% bleach/90% water solution** (household bleach containing less than 10% sodium hypochlorite.
3. **Do not use** ammonium chloride based cleaning fluids.
4. **Wipe away from connector plug.** Do not submerge or immerse sensor or connector plug.
5. **Allow to completely dry** before next use.
6. **Confirm cleaning adequacy** by visually inspecting for residual soil. If residual soil is present, repeat cleaning until residual soil is no longer present. If residual soil is unable to be removed, properly and safely dispose of device.

   Note: To minimize cable deterioration when cleaning the cable, gently wipe away from the plug end towards the sensor end.

   Clean the device promptly after use to prevent drying of soil and/or contaminants.

Nonin.com

United States
info@nonin.com
+1.763.553.9968

International
info@nonin.com
+31 (0)13 - 45 87 130

The only way to ensure that clinicians get Nonin's tested SpO_2 accuracy and consistency in the widest range of patients and settings[1] is to use Nonin PureLight® sensors with your Nonin PureSAT® pulse oximeters.

For more information about Nonin's sensor portfolio go to Nonin.com/sensors

THIS GUIDE IS FOR REFERENCE ONLY. Refer to the Instructions for Use for complete information, warnings, cautions and specifications for the product you are using.

℞ only

1 Nonin Medical, Inc. Data on File.

© 2023 Nonin Medical, Inc. All trademarks are the property of Nonin Medical, unless otherwise noted.
M-23-095-01