# WHERE COMFORT MEETS ACCURACY

## 6000C Series

Disposable Cloth Pulse Oximetry Sensors

Comfortable Design

Accurate Technology

Sizes for All Patients

Designed with an inclusive cable, sensor, and adhesive cloth wrap, Nonin 6000C Series disposable cloth pulse oximetry sensors provide ultimate comfort for patients requiring extended $SpO_2$ and pulse rate monitoring and secure placement. The sensor design features a stretch, tear-resistant cloth for easier placement and fit on the patient, especially for hard-to-fit patients such as infants and neonates, supporting accurate[1] readings by keeping the sensor in the proper position.

Each 6000C Series disposable sensor features Nonin PureLight® technology and Nonin PureSAT® signal processing to provide accurate $SpO_2$ and pulse rate readings, even in motion[2] or low perfusion.[3]

NONIN

# Measurements You Can Trust.

With sizes from neonate to adult, you can count on a proper fit for an accurate reading.[1]

Single-use sensors are ideal for situations where risk of cross contamination is high.[4,5]

Special adhesive allows the sensor to be repositioned multiple times.

Illustrated finger guide ensures easy and accurate placement by caregiver or patient.

Tear resitance increases the number of times the sensor can be repositioned.

Designed with a breathable cloth material for patient comfort: latex free and fully compliant with REACH, RoHS, and PFAS requirements.[6]

## For Patients of Many Sizes and Clinical Presentations

Available in four sizes ranging from neonate to adult, applied to finger or toe.

6000CA Adult: (>30kg/>66lbs)

6000CP Pediatric: (>10kg/>22lbs)

6000CI Infant: (>2kg/>4lbs)

6000CN Neonate: (<2kg/<4lbs)

Cable lengths ranging from 1m, 3m, 6m, and 9m.

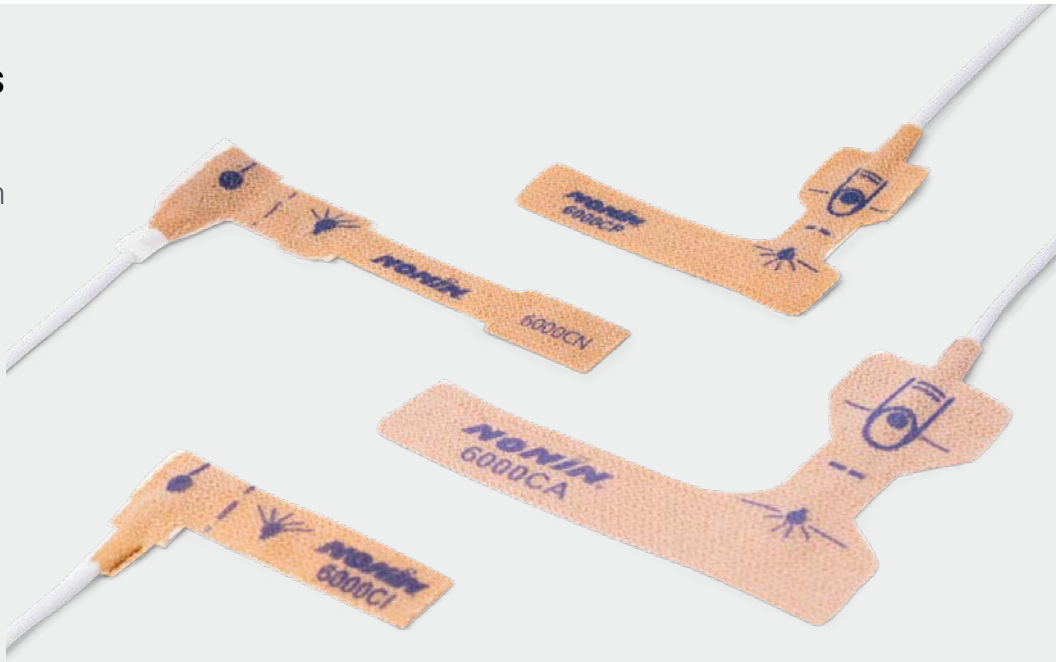


1,2,3,6. Nonin Medical, Inc. Data on File.
4. Chambers, C.E., Eisenhauer, M.D., McNicol, L.B., Block, P.C., Phillips, W.J., Dehmer, G.J., Heupler, F.A. and Blankenship, J.C. (2006), *Infection control guidelines for the cardiac catheterization laboratory: Society guidelines revisited*†. Cathet. Cardiovasc. Intervent., 67: 78-86. https://doi.org/10.1002/ccd.20589
5. Nandy P, Lucas AD, Gonzalez EA, Hitchins VM. *Efficacy of commercially available wipes for disinfection of pulse oximeter sensors*. Am J Infect Control. 2016;44(3):310-313. doi:10.1016/j.ajic.2015.09.028

Accuracy tested with Nonin Models 2500, 7500, 3150, and OEM III Module.

**Nonin Medical, Inc.**
13700 1st Avenue North, Plymouth MN • 55441-5443 • USA
**Tel:** +1.763.553.9968 *OR* +1.800.365.8874
**Email:** info@nonin.com

NONIN
nonin.com

©2026 Nonin Medical, Inc. All copyrights and trademarks are the property of Nonin Medical, Inc. unless otherwise noted and or used under license. All rights reserved. M-26-020-01

Rx Only