

# Nonin Model 7500 Tabletop Pulse Oximeter with Hybrid Averaging™


## Competency Checklist

### Competency Objectives

To demonstrate proficiency in the clinical applications of monitoring the patient, set-up, and proper operation of the Nonin Model 7500 Pulse Oximeter with Hybrid Averaging.

### Participant will be required to demonstrate the following:

- Device set up for patient use
- Attachment of sensor the patient
- Monitoring the patient
- Common troubleshooting techniques

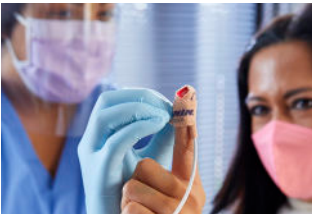

### Resources



Product  
information



Product  
training

| Quick Setup                                                                              | Completed | Initials |
|------------------------------------------------------------------------------------------|-----------|----------|
| Unpack and set up the Model 7500 to begin charging                                       |           |          |
| Confirm charging indicators and confirm amount of time until full charge                 |           |          |
| Once charged, turn on the Model 7500                                                     |           |          |
| Demonstrate how to set the Model 7500 to the user-defined defaults                       |           |          |
| Demonstrate how to set patient security mode                                             |           |          |
| Demonstrate how to set data collection and download                                      |           |          |
| Monitoring the Patient                                                                   | Completed | Initials |
| Place sensor                                                                             |           |          |
| Attach sensor                                                                            |           |          |
| Review and describe each indicator on the display                                        |           |          |
| Troubleshooting                                                                          | Completed | Initials |
| Demonstrate how to get back display when SpO <sub>2</sub> and pulse rate are not showing |           |          |
| Demonstrate how to silence alarms                                                        |           |          |
| Optional Features                                                                        | Completed | Initials |
| Change the Model 7500 from Standard/Fast Averaging to Hybrid Averaging                   |           |          |
| Describe what each error code means (E01 and E04)                                        |           |          |
| Explain and demonstrate how to clean the device                                          |           |          |
| Describe how to store the device after use                                               |           |          |

Employee Signature: \_\_\_\_\_ Date: \_\_\_\_\_

Evaluator Signature: \_\_\_\_\_ Date: \_\_\_\_\_

For additional information, visit [nonin.com/products/7500/](https://nonin.com/products/7500/)

